Certificate of Analysis

ILS Laboratories
8222 Vickers St, Suite 106, San Diego, CA 92111
(619) 329-3999 | ils-lab.com

GLP-2 TR - 30mg

Tested for: Klow.bio
3838 N Ravenswood Ave, Chicago, Illinois, 60613-5651 | https://klow.bio


PASS

Scan to verify authenticity at ils-lab.com
Access Code: DM2KKDXR

COA #:	**COA-2026-VYDDYS**	Analysis Date:	**09/23/2026**
Lot Number:	**KB-52383**	Appearance:	**Good**
Accession #:	**ACC-2026-18995**	Sample Matrix:	**Lyophilized**
Labeled Content:	**30mg**	Volume:	**3mL**
		Date Received:	**09/09/2026**

Method: **Purity, Identity & Quantitation (HPLC)**

Identity GLP2-TR 30mg | Peptide Purity **99.77%** | Fentanyl Free

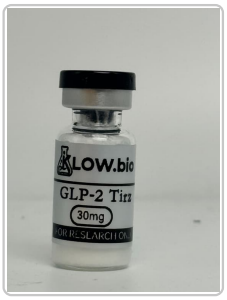


Tirzepatide 30mg - KB-52383

Purity, Identity & Quantitation (HPLC)

Analyte	Specification	Result	Unit	Status
Peptide Purity (HPLC)	>= 95.0%	**99.77%**	%	**PASS**
Net Peptide Content	Report Only	**31.15**	mg	N/A
Identity (HPLC-RTM)	GLP-2 TR	**Confirmed**	-	**PASS**
Fentanyl Screen	Immunoassay, 50 ng/mL cutoff	**Not Detected**	-	**PASS**

HPLC Chromatogram

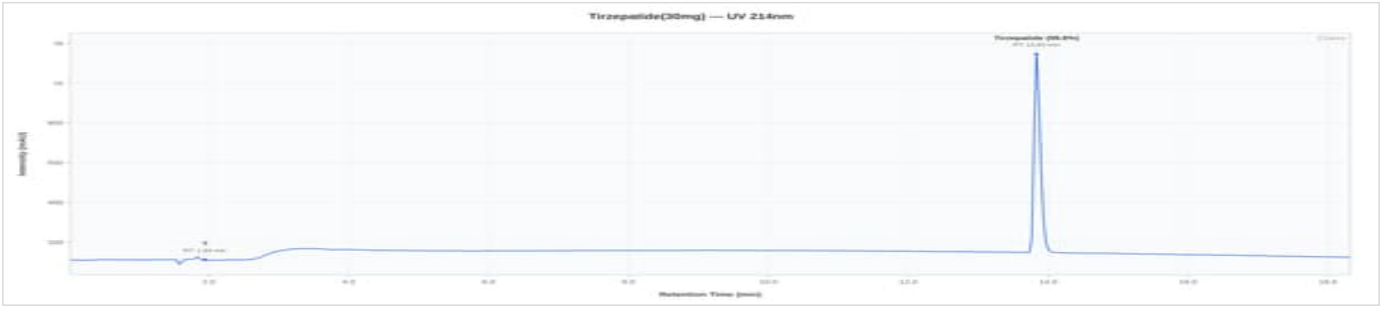

Tirzepatide 30mg - KB-52383: UV Chromatogram

Notes & Methodology

1. Date Tested: 09/23/2026. Methods: Purity, Identity & Quantitation (HPLC).
2. The sample was confirmed to be Tirzepatide by HPLC. Identification by chromatographic retention time comparison with a reference standard.
3. Peptide purity determined by RP-HPLC area normalization at 214 nm. Value represents the percentage of the target peptide relative to all peptide-related peaks. Non-peptide process-related impurities, if detected, are excluded from the calculation.
4. Accreditation Scope: ILS Laboratories maintains ISO/IEC 17025 accreditation for activities listed in its published PJLA scope. Peptide testing reported on this certificate is performed for Research Use Only.
5. This certificate reports analytical results for the sample(s) submitted to ILS Laboratories for testing. All sample identifications, product names, brand names, lot/batch numbers, and labeled content are provided by the submitting party and have not been independently verified. Results reflect only the analytical testing of the specific sample(s) provided and do not constitute an evaluation or endorsement of the manufacturer's processes, quality systems, or overall production. ILS Laboratories makes no representations regarding the intended use, safety, efficacy, regulatory status, or intellectual property ownership of any materials tested.

Issued by ILS Laboratories
(619) 329-3999
ils-lab.com

Dr. Greg Kalyuzhny
Lab Director
09/23/2026

COA #: **COA-2026-VYDDYS**
Access Code: **DM2KKDXR**
Verify: portal.ils-lab.com/verify/tem9mOLw0bxn39j3
Issued: 09/23/2026